



Data Conditioning


Supported by FFT Spectral Analysis, Time-Stamp, Order-Tracking, Sine Reduction & Basic Signal-Conditioning support data conditioning features. Data Conditioning supports functions to control and process data using a logic gate structure.

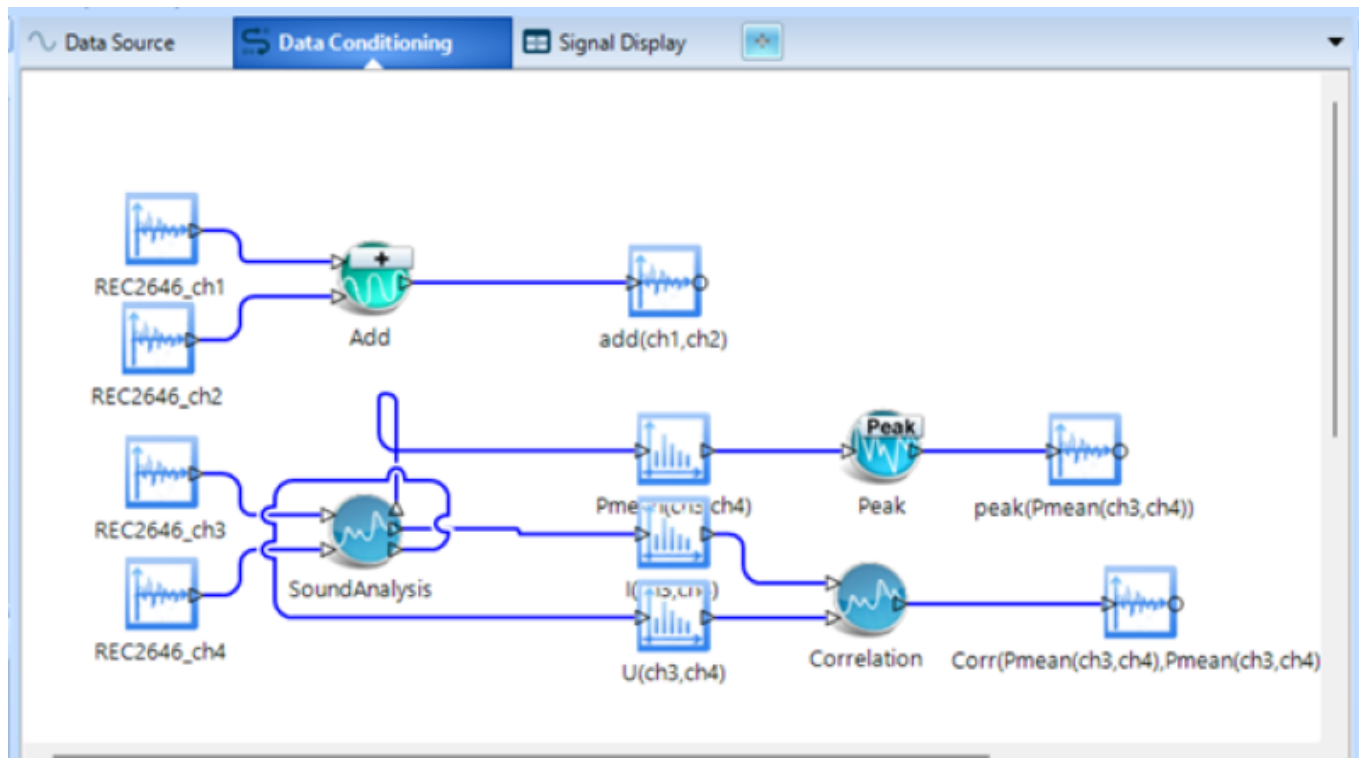


Follow the guided steps below to understand and use the data conditioning functionality in Post Analyzer

Data conditioning tabs can be opened through the Setup → Data Conditioning dropdown, or the user can press Ctrl+Shift+D.

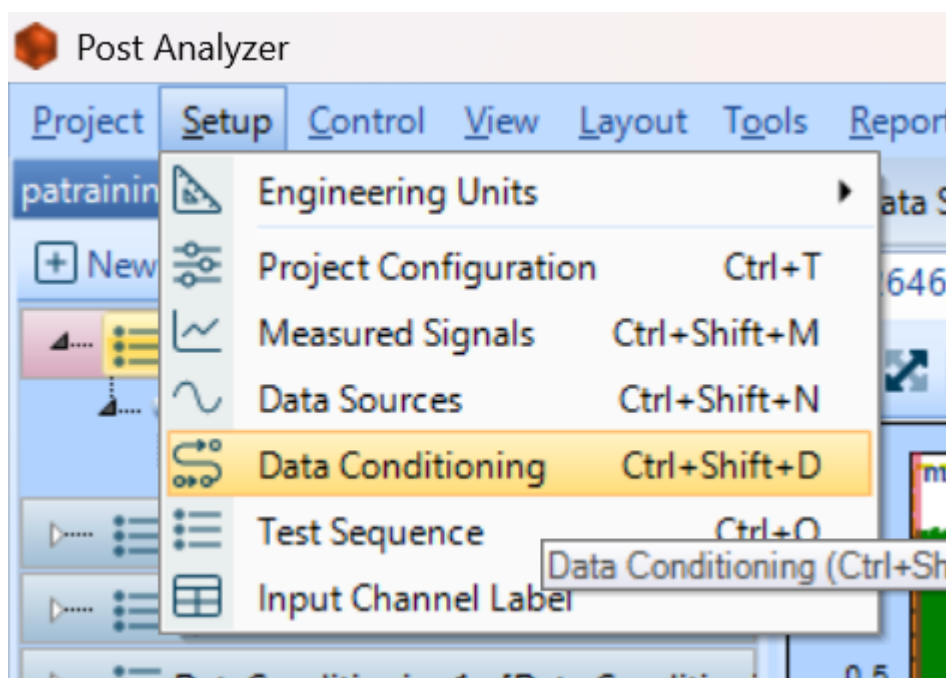

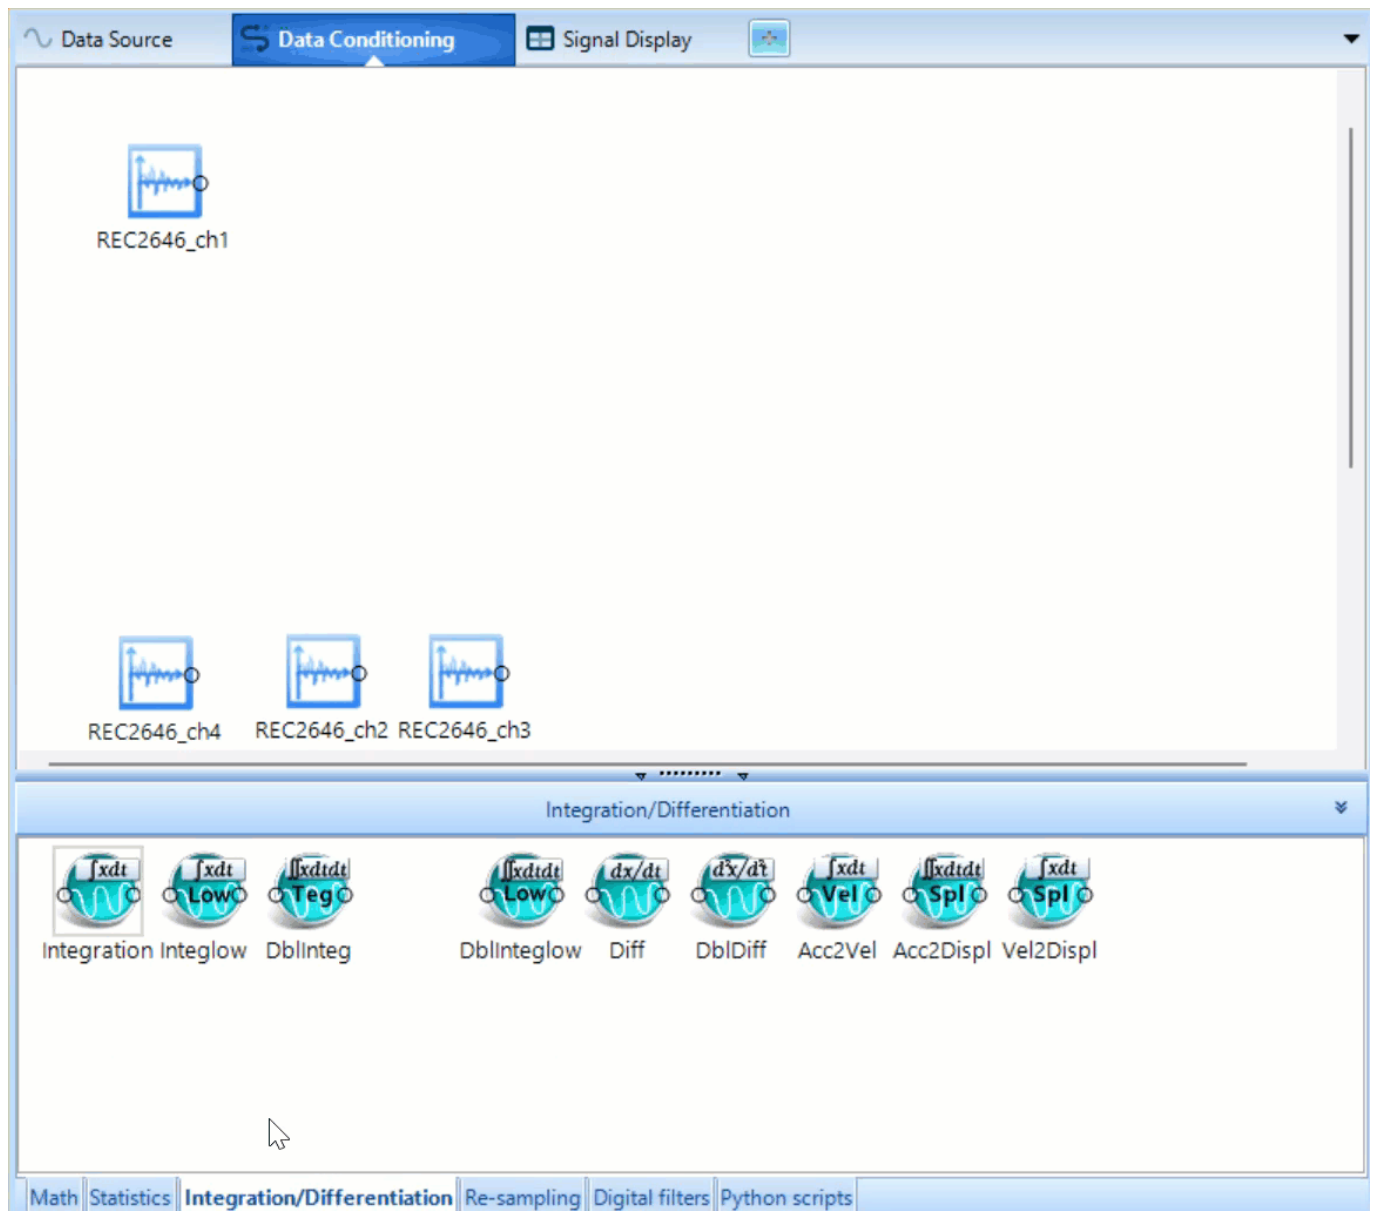****Simple Data Conditioning Demonstration****

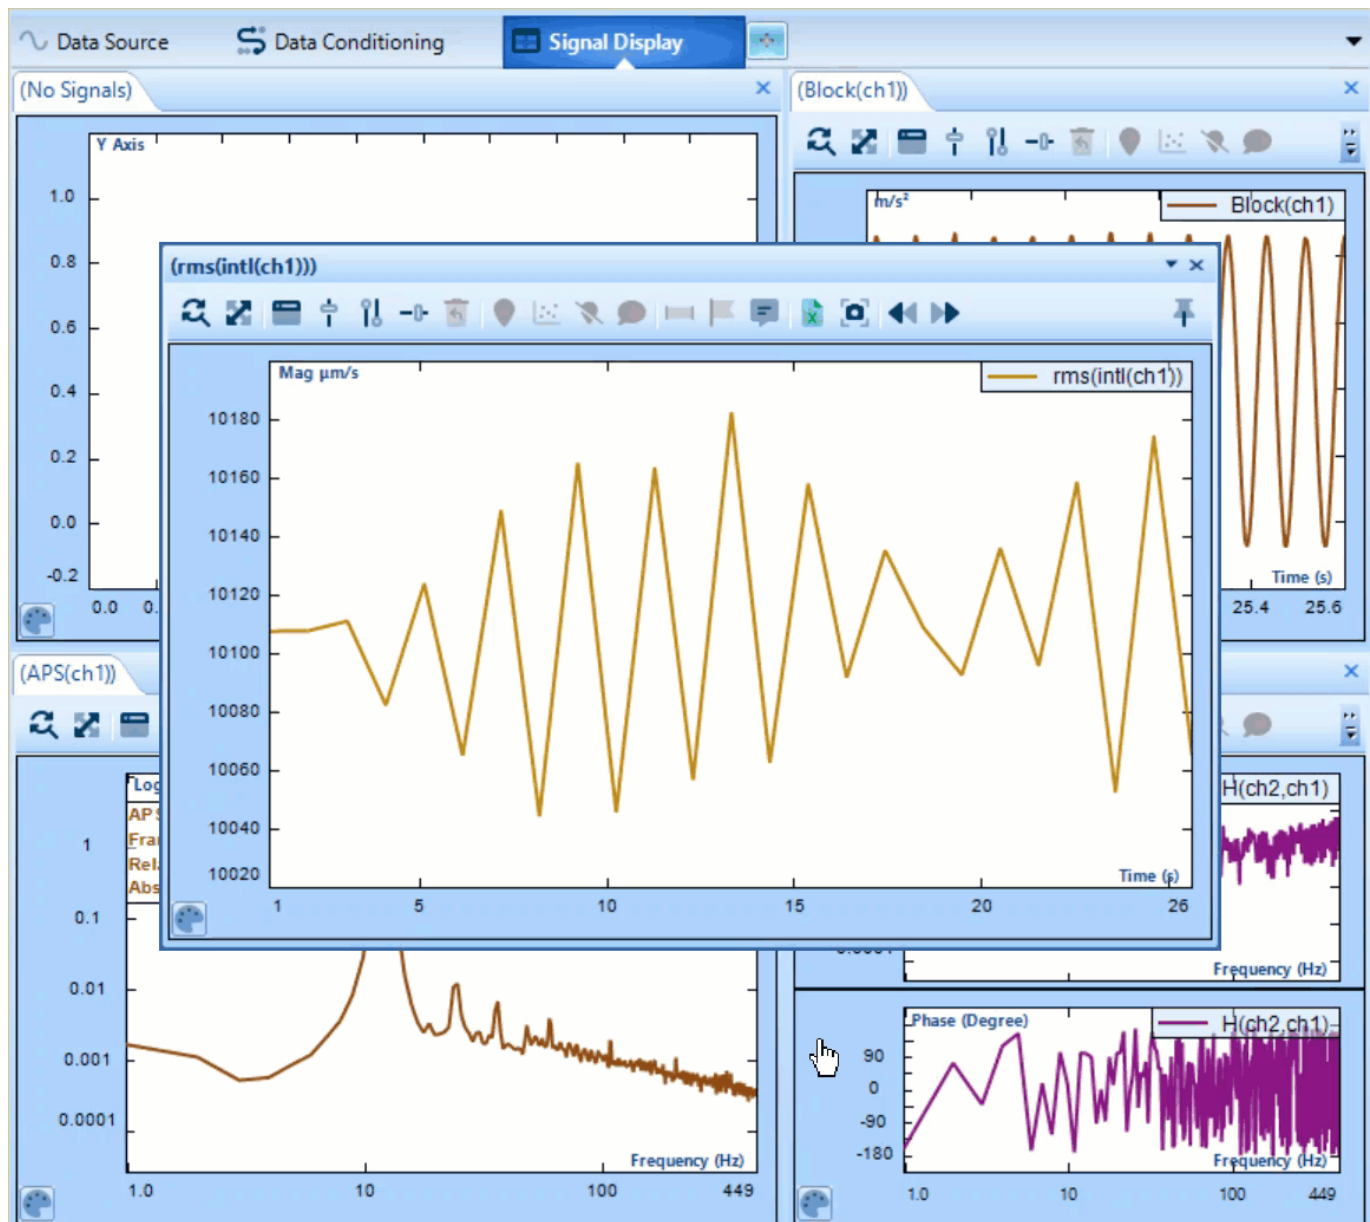

From:

<https://help.go-ci.com/> - **Crystal Instruments Help**

Permanent link:

<https://help.go-ci.com/pa-data-conditioning?rev=1769806422>

Last update: **2026/01/30 20:53**