


Spider Check List

This window allows the user to confirm all the settings and make any last-minutet changes. The window has sections for pre-test settings, shaker information, test level and duration information, and input channel configuration. Most of these channels can be edited by clicking on the blue underlined text. There is also a sectin for ading custom report fields and a test description.

Test > Checklist or **Ctrl+Shift+K** to open the window.

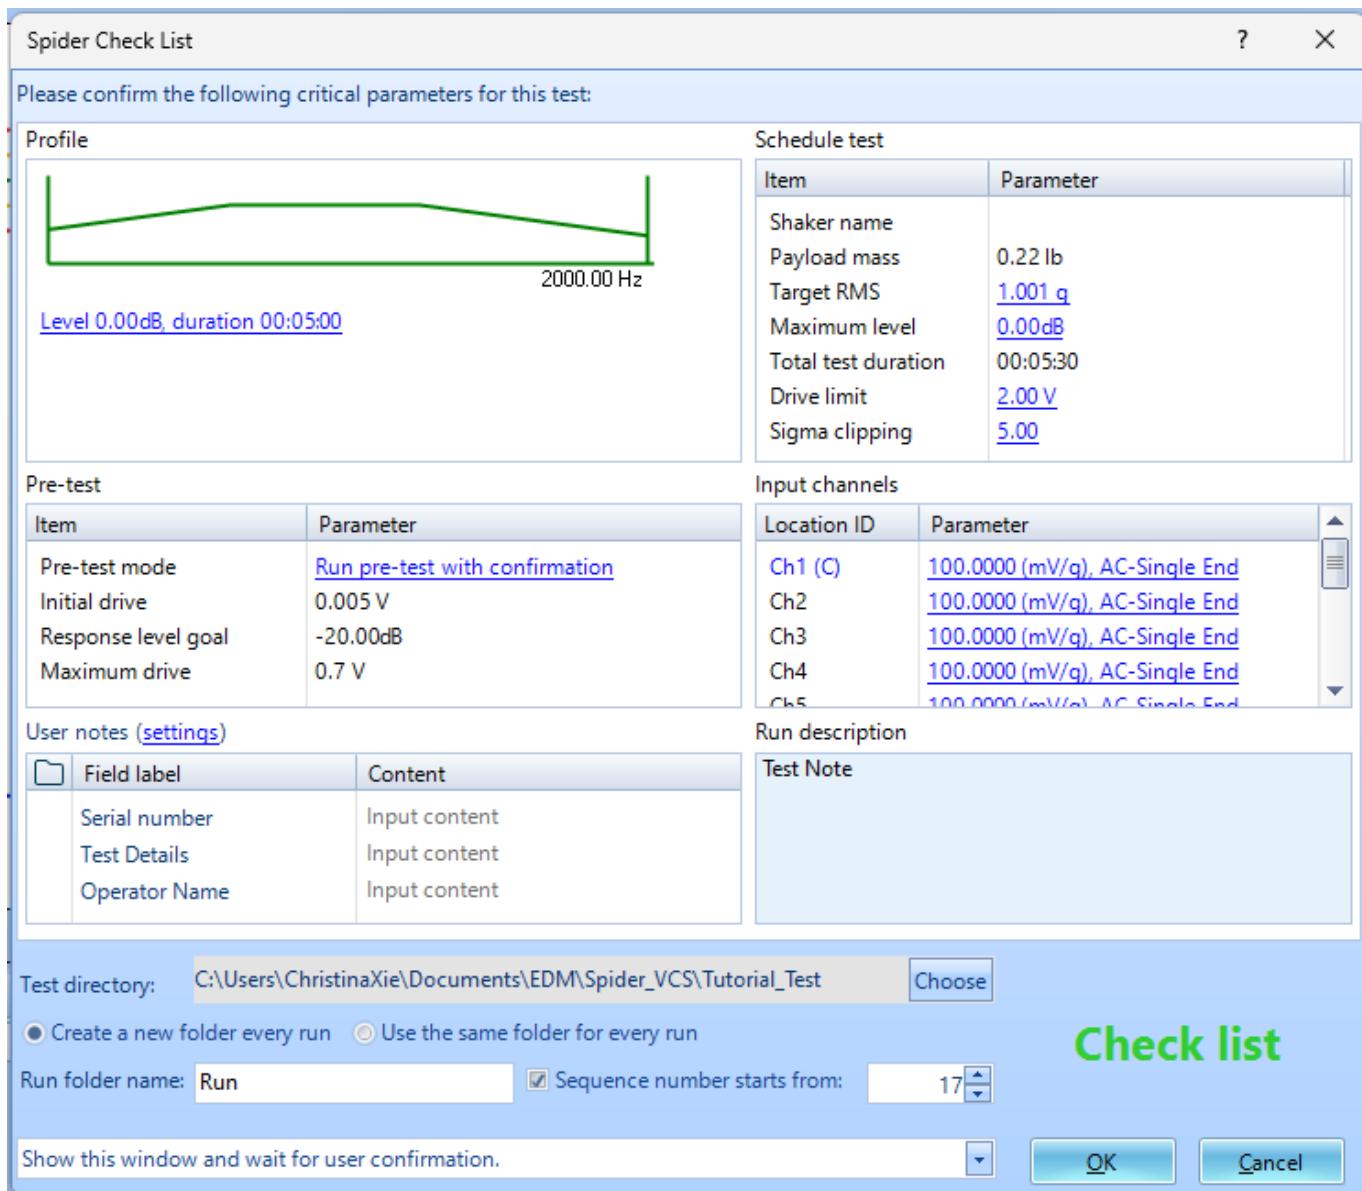

Run Schedule, Test Profile, Pre-test Parameters sections can all be found in the control panel clicking the **Config** button.

Setup > Input Channels or **Ctrl+I**.

Tools > User Notes Settings. It is where you can input your key data values that you want to include before running. The Field Labels here are customizable, so if you have more data values you would like to add, you can click **Insert** and then type in the textbox.

From:
<https://help.go-ci.com/> - **Crystal Instruments Help**

Permanent link:
<https://help.go-ci.com/vcs:spiderchecklist?rev=1734118728>

Last update: **2024/12/13 19:38**