


VCS UI New Test Wizard

When starting the software or creating a new test type you will be presented with the following screen:

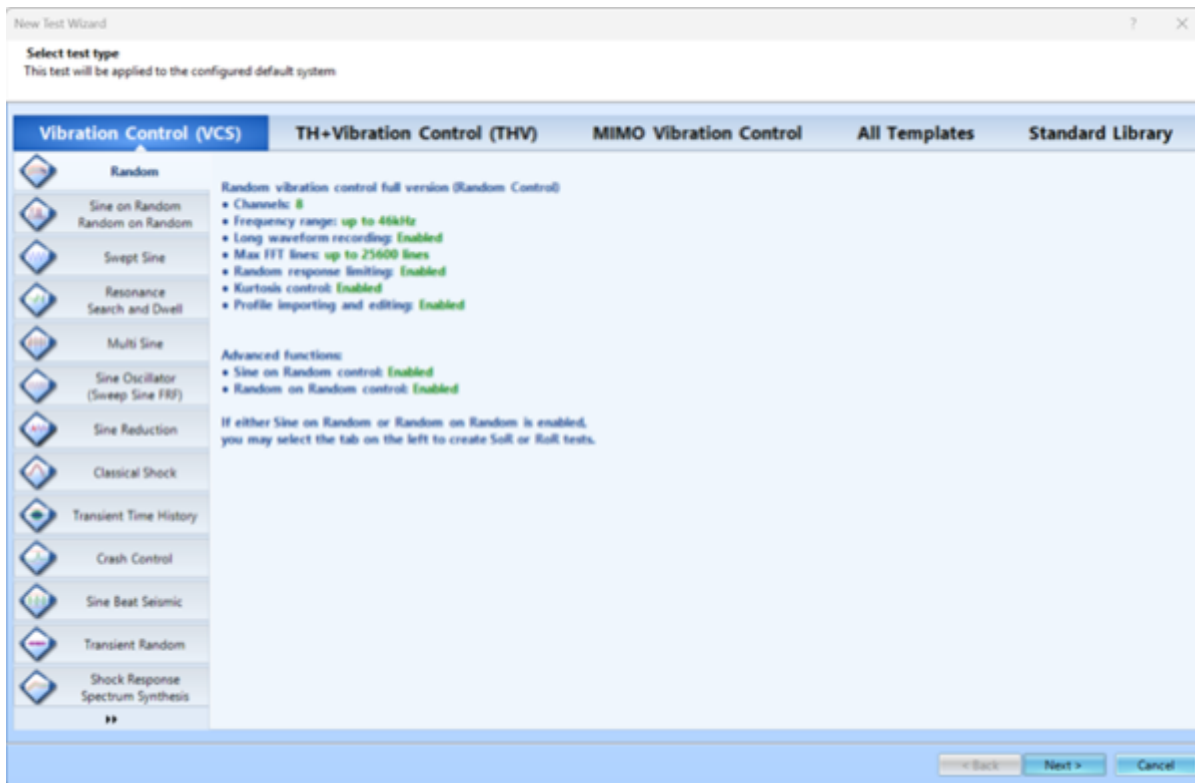

Ribbon

Vibration Control (VCS)

Standard single input single output closed loop control of a shaker


TH+Vibration Control (THV)

Allows for temperature, Humidity & Vibration control simultaneously

MIMO Vibration Control


Multiple Input Multiple Output and Multiple Exciters Single Axis (MESA) control types run through this panel

Allows for multiple control outputs to be used to control several degrees of freedom for UUT or greater force transfer to objects too large to be tested properly by a single shaker unit.

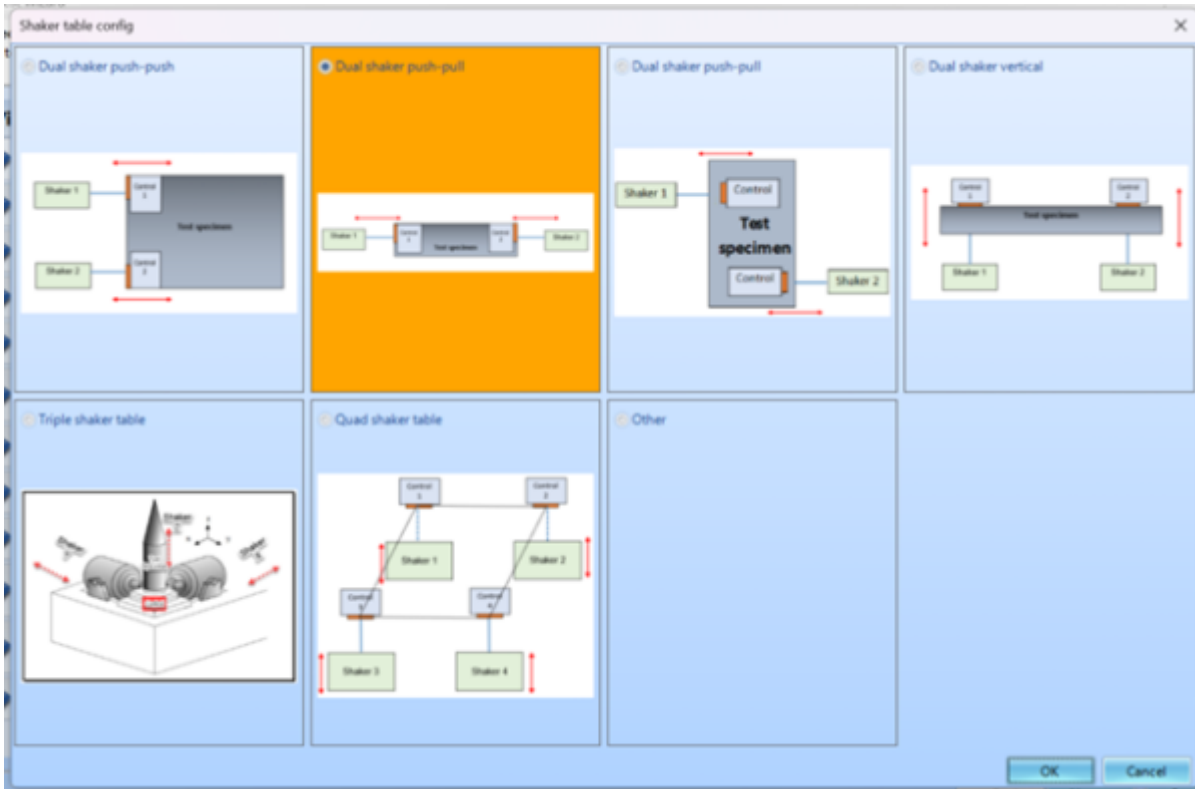

IF MIMO VC is selected, once test type is selected and you click next; you will be presented with the screen above to select the shaker setup you are working on.

Panels

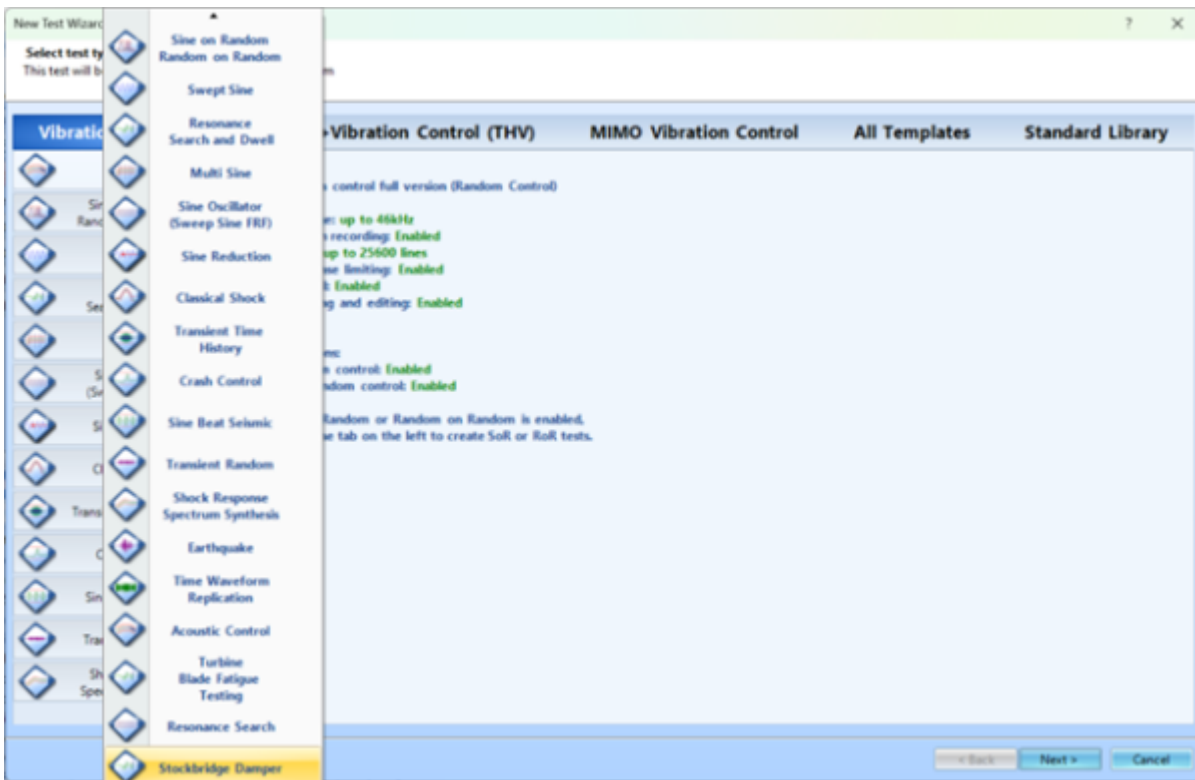

Test Types

The most used test types are Random, Sine Sweep & SRS

Random

Random excitation is often used to simulate real-world vibration. The purpose of the random vibration control system is to generate a true random drive signal such that, when the signal is applied via an amplifier/shaker to the device under test, the resulting shaker output spectrum will match the user-specified test profile. VCS also has the capability to perform Sine on Random (SoR) and Random on Random (RoR) testing.

Swept Sine

Unlike Random testing which generates many frequencies at once over the band of interest, Swept Sine testing generates energy at one frequency and sweeps this frequency through a preset range.

Classic Shock

A Shock test outputs a series of pulses to excite the structure under test. The response is measured at one or more locations on the structure and a spectral analysis is used to determine its response and resonance characteristics. This pulse response approximates the impulse response, the theoretical response to an infinitely tall and narrow spike function with an area of unity.

THV

Uses a limited set of tests available in VCS.

MIMO Vibration Control

Uses primarily the same testing types as VCS with custom features for MESA & MIMO applications. Additionally, it includes options for 3 Axis 6-DOF testing. Has a specialized Time waveform Replication with an iterative approach.

Test Description

Fill in the basic information for this test
Note: you will be able to search for this test by "Test name" or "Test description".

Create a new Random test: Random Test

Test name: Random Test Append the sequence number

Test description:

Use the default libraries of the previous test of the same type. If default libraries were not applied before the manufacturing settings will be used.

Create test by using a template.

Select	Template name	Description
--------	---------------	-------------

Optimize test parameters for: Electrodynamic shaker Hydraulic shaker

Spider system: SYS_1033504

Test directory: C:\Users\ReidGarcelon\Documents\EDM_VCS\Spider_VCS\Random Test

Create new run folder for each run

< Back Create test Cancel

Test name can be defined by user needs. Shaker Type will be set to either Electrodynamic Shaker or

Hydraulic Shaker depending on test setup. Spider system must be connected directly to PC conducting tests. Spiders are only capable of conducting tests for one user at a time.

From:
<https://help.go-ci.com/> - **Crystal Instruments Help**

Permanent link:
<https://help.go-ci.com/vcs:ui-overview:new-test-wizard?rev=1771358575>

Last update: **2026/02/17 20:02**