


Loading and Unloading Data from CoCo

The screenshot displays the Carrier Vibration Analysis Tool interface. The top navigation bar includes tabs for Review, Data Collector, Tool, Setup, System, and Off Route. The Data Collector tab is active, showing icons for Load and Unload, which are highlighted with a red box. Below this are sections for Param Sets, Tacho Sets, Sensor Sets, and Alarm Sets. The main window shows a synchronization wizard titled "Carrier Vibration Analysis Tool Synchronization Wizard | Database: smart2". The wizard prompts the user to "Please select to synchronize with a CoCo device or a folder". The "File folder (Name is CoCo-80)" option is selected and highlighted with a red box. A red arrow points to the "CoCo 70x/80x" option under the "Target Device" section, which is also highlighted with a red box. A red text annotation "select correct device type" is positioned above the arrow. The wizard also displays "Supported Device Type: Card and Normal" and instructions to click the [Next] button to continue. Navigation buttons for "< Back", "Next >", and "Cancel" are at the bottom.

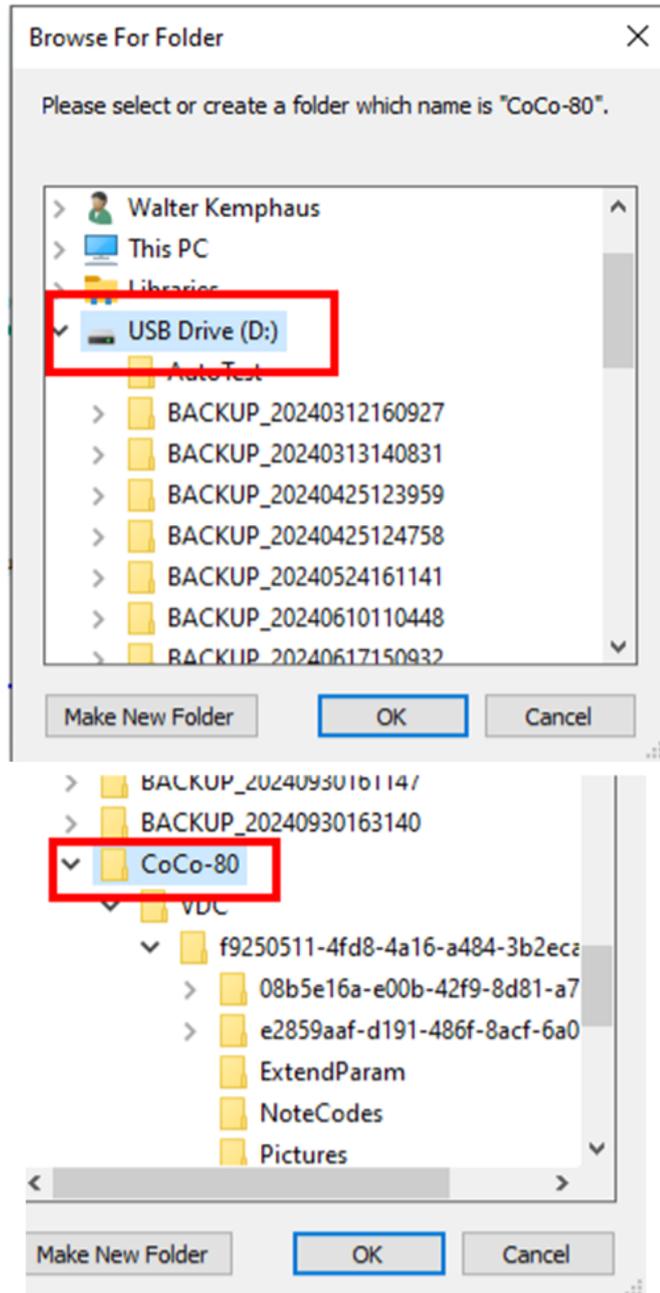

In VDS, click **Data Collector** > in the **Devices** menu, click **Load** > Click **CoCo device** > **Select** the Device you are using > Select the card name > Click **Next** > Click the **Browse** button > select the proper path > **choose the folder CoCo-80** > Click **OK**.

To unload, follow the same steps from above after clicking the **Unload** button from the Devices menu.

From:
<https://help.go-ci.com/> - **Crystal Instruments Help**

Permanent link:
<https://help.go-ci.com/vds:transfer?rev=1734725007>

Last update: **2024/12/20 20:03**